


Group	Test	N	TP	FP	TN	FN	Sensitivity [95% CI]	Specificity [95% CI]
All								
	Bio-Rad Total Ab	398	79	0	298	21	0.79 [0.70–0.86]	1.00 [0.99–1.00]
	Darui IgG	400	72	7	293	28	0.72 [0.63–0.80]	0.98 [0.95–0.99]
	Darui IgM	400	74	4	296	26	0.74 [0.65–0.82]	0.99 [0.97–0.99]
	Epitope Dx IgG	389	73	6	287	23	0.76 [0.67–0.83]	0.98 [0.96–0.99]
	Epitope Dx IgM*	175	49	1	80	45	0.52 [0.42–0.62]	0.99 [0.93–1.00]
	EuroImmune IgA-S	387	80	10	279	18	0.82 [0.73–0.88]	0.97 [0.94–0.98]
	EuroImmune IgG-S	388	55	2	294	37	0.60 [0.50–0.69]	0.99 [0.98–1.00]
	EuroImmune IgG-N	392	70	9	286	27	0.72 [0.63–0.80]	0.97 [0.94–0.98]
	NovaTec IgA	393	70	2	293	28	0.71 [0.62–0.79]	0.99 [0.98–1.00]
	NovaTec IgG	392	62	3	293	34	0.65 [0.55–0.73]	0.99 [0.97–1.00]
	NovaTec IgM*	174	41	0	83	50	0.45 [0.35–0.55]	1.00 [0.96–1.00]
	SD Bio Total Ab	400	80	2	298	20	0.80 [0.71–0.87]	0.99 [0.98–1.00]
	Teco IgG*	180	89	37	46	8	0.92 [0.85–0.96]	0.55 [0.45–0.66]
	Teco IgM	396	64	1	295	36	0.64 [0.54–0.73]	1.00 [0.98–1.00]
	Wantai IgM	397	77	8	291	21	0.79 [0.69–0.86]	0.97 [0.95–0.99]
	Wantai Total Ab	397	86	3	295	13	0.87 [0.79–0.92]	0.99 [0.97–1.00]

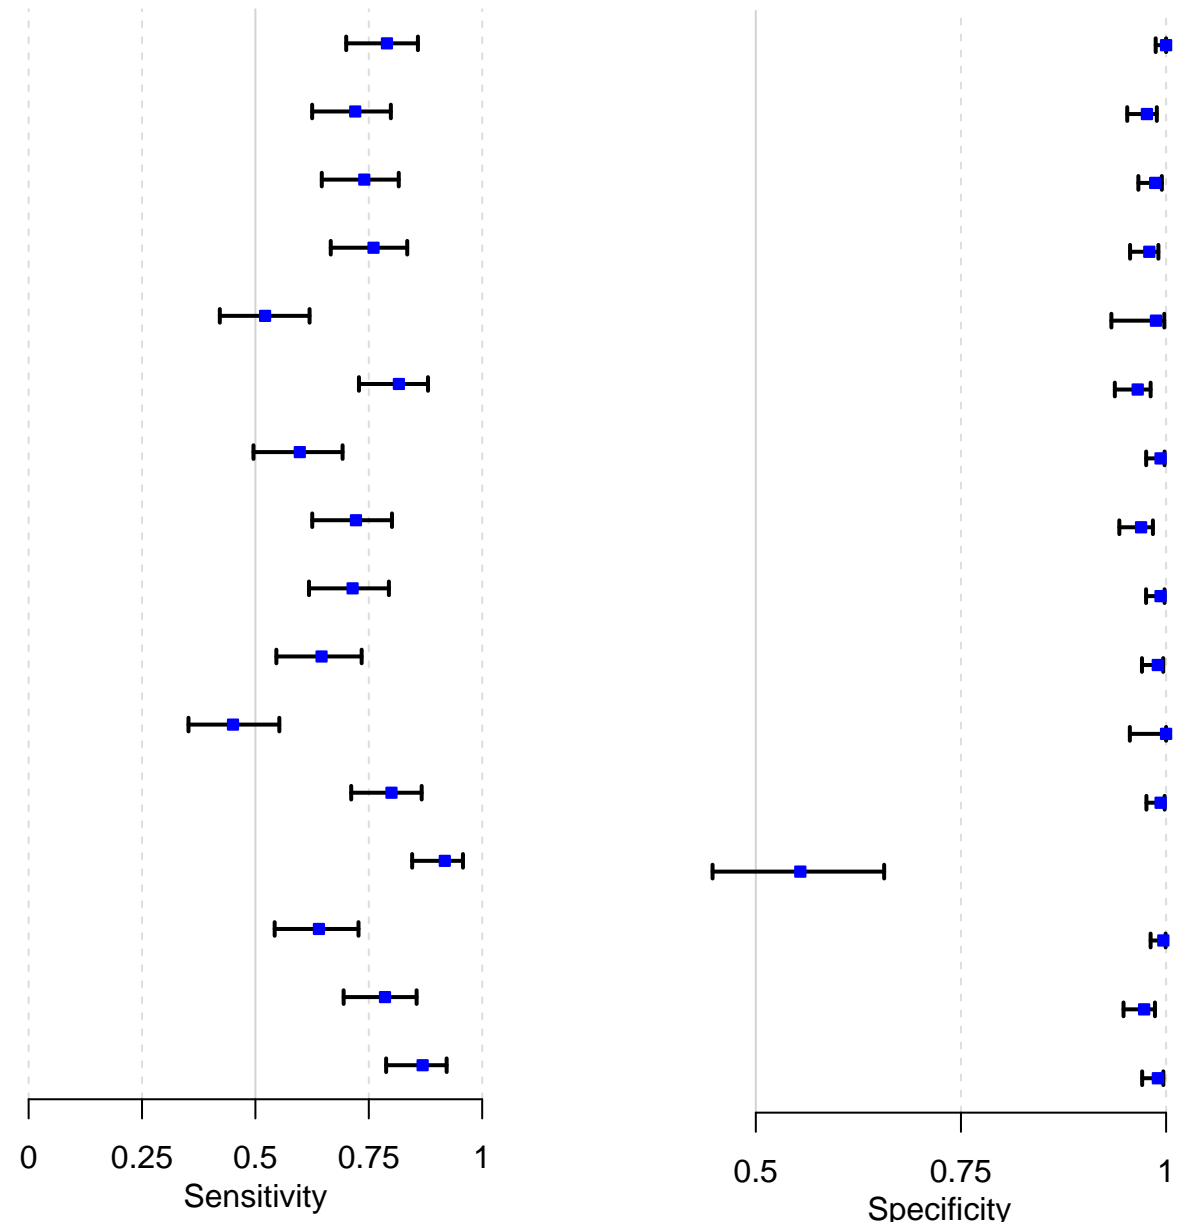

* did not pass to full panel.